

Upgrade of the GADAST detector by 16 LaBr₃ scintillator detectors*

I. Mukha¹, V. Dunin², A. Fomichev³, S. Krupko³, A. Bezbakh³, S. Baraeva³, A. Gorshkov³, A. Knyazev³, P.G. Sharov³, C. Scheidenberger¹, H. Simon¹, and R. Slepnev³

¹Helmholzzentrum GSI, Darmstadt, Germany; ²Veksler and Baldin Laboratory of High Energy Physics, JINR, Dubna, Russia; ³Flerov Laboratory of Nuclear Reactions, JINR, Dubna, Russia

The GAMMA-ray Detector Around Secondary Target (GADAST) can be used in the middle of the FRS and Super-FRS fragment separators [1], which helps to exploit their unique performance in a separator–high-resolution-spectrometer mode. The main part of the GADAST consisted of 64 large-size scintillating CsI(Tl) crystals in production at JINR, Dubna. The GADAST demonstrator of 16 such detectors has been successfully tested at FRS GSI in 2012 [2]. In order to upgrade the GADAST at forward angles, we build in addition an array of 16 LaBr₃ scintillator crystals (cylinders of 1x4 inches) with improved light readout and electronics being able to work at high counting rates up to 10^6 s⁻¹ with the energy resolution of 3 %.

During the upgrade of GADAST, the 64 CsI(Tl) detectors have received a new mechanical structure (4 crystals in one cluster), which allows for various geometries of the GADAST setup depending on experimental task. Each crystal is coupled with a photo multiplier tube (PMT) either of R7600U-300 Hamamatsu (40 units in total) or 9106SB ET (24 units) types. The in-house developed electronics, being operated at +12 V only, provides a high-voltage (HV) bias, strong amplification of the detector signals and their shaping as well as logical signals via a delay line of 0.8 μ s. However, the CsI(Tl) detectors work at counting rates $\leq 3 \times 10^4$ s⁻¹, which is not sufficient at forward angles where counting rates are very high.



Figure 1: The components of the LaBr₃ detector.

Scintillation LaBr₃ crystals are much faster and provide better energy resolution. Thus we have developed a cluster of 16 detectors with LaBr₃ crystals. Dimensions of the crystals were chosen of 2.5 cm in diameter (in order to minimize a Doppler broadening of detected γ -rays) and 10 cm in length (to detect γ -rays up to energies of 10-20 MeV). We have chosen a PMT type 9142SB ET with an enforced voltage divider and a plate with combined HV-bias, preamplifier of dinode signals and shaper (similar to those developed for the CsI(Tl) detectors [2]). The components of the

disassembled LaBr₃ detector are shown in Fig. 1.

Performance of the developed detectors is illustrated in Fig. 2, where the γ -ray spectrum measured from ¹³⁷Cs source shows the energy resolution of 3.0(1) % (the full width at half maximum (FWHM) of the peak of 662 keV γ -rays measured with a shaping time of 0.5 μ s). The obtained energy resolution is even better than the resolution of 3.4 % reported by the St. Gobain manufacturer. The low energy detection threshold of \sim 50 keV is achieved.

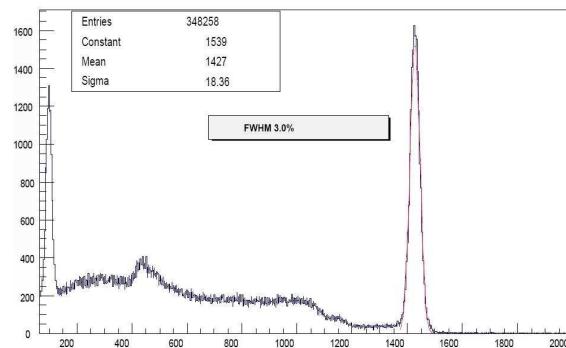


Figure 2: The γ -ray spectrum of a standard ¹³⁷Cs source measured with the developed LaBr₃ detector. The right peak corresponds to 662 keV γ -transitions.

The detector GADAST is ready for experiments since 2014. We plan to use it at the new ACCULINNA-2 (JINR, Dubna) fragment separator [3] and later at the FRS and the Super-FRS fragment separators [4]. Applications of the developed detectors are possible also for the other experiments of the NUSTAR collaboration at FAIR.

References

- [1] I. Mukha *et al.*, "Gamma detector around a secondary target (GADAST) at the middle of the fragment separator FRS", LoI 49 to the G-PAC GSI (2010), unpublished.
- [2] I. Mukha *et al.*, "First Operation of the GADAST, GAMMA-ray Detector Around a Secondary Target in the Middle of FRS: Measurements of inelastic Scattering of ¹⁷Ne", GSI Scientific Report 2012, PHW-ENNA-EXP-45, p.175, <http://repository.gsi.de/record/52876>.
- [3] A.S. Fomichev *et al.*, "Long-range plans for research with radioactive ion beams at JINR", JINR Communication E7-2012-73, Dubna, 2012.
- [4] "Scientific program of the Super-FRS Collaboration: Report of the collaboration to the FAIR management", GSI Report 2014-4, doi:10.15120/GR-2014-4.

* Work supported by the grants BMBF GSI-JINR and Helmholtz-Rosatom for FAIR.

